# Cibinetide 10 mg — 10mg

PASS

Verum Analytical · Peptide & Compound Testing Services
3020 E Camelback Rd, Suite 397, Phoenix, AZ 85016 · +1 (480) 393-4256 · verumanalytical.com

**Tested for: BH Lab**
1445 E Madison St, Brownsville, TX 78520 | beyondhealthlab.com

| | | | |
|---|---|---|---|
| COA # | **COA-2026-VA-ARA290-10** | Method | **Certificate of Analysis** |
| Lot number | **VA-ARA290-10** | Analysis date | **2026-09-08** |
| Concentration | **10mg** | Appearance | **Good** |
| Received | **2026-09-07** | Volume | **3ml** |

IDENTITY
**Cibinetide 10 mg**

PURITY
**>99.80% + 0.18%**

● VERIFIED AT SOURCE  Lot **VA-ARA290-10** · authentic record held by Verum Analytical

SCAN TO VERIFY

## QC CERTIFICATE OF ANALYSIS

| ANALYTE | SPECIFICATION | RESULT | UNIT | STATUS |
|---|---|---|---|---|
| Chromatographic Purity | — | >99.80% + 0.18% | % | PASS |
| Assay | — | 10.80 mg | mg | PASS |

## HM HEAVY METALS ANALYSIS (ICP-MS)


| TEST | SPECIFICATION | RESULT | STATUS |
|---|---|---|---|
| Chromium (Cr) | — | ND | PASS |
| Arsenic (As) | — | ND | PASS |
| Cadmium (Cd) | — | ND | PASS |
| Lead (Pb) | — | ND | PASS |
| Mercury (Hg) | — | ND | PASS |

## 5 MICROBIOLOGY

| PARAMETER | METHODOLOGY | ACCEPTANCE / LIMIT | RESULT |
|---|---|---|---|
| Endotoxins | LAL | Pass/Fail criteria based on the USP/FDA threshold of 5 EU/kg (350 EU total for a 70 kg adult) | PASS - <0.05 EU/mg |
| Sterility | USP <71> | — | PASS - No microorganisms present in sample tested. |
| ScanRDI Sterility Test | ScanRDI | — | Pass |

## HPLC CHROMATOGRAM

HPLC chromatogram — ara 290 · 214 nm

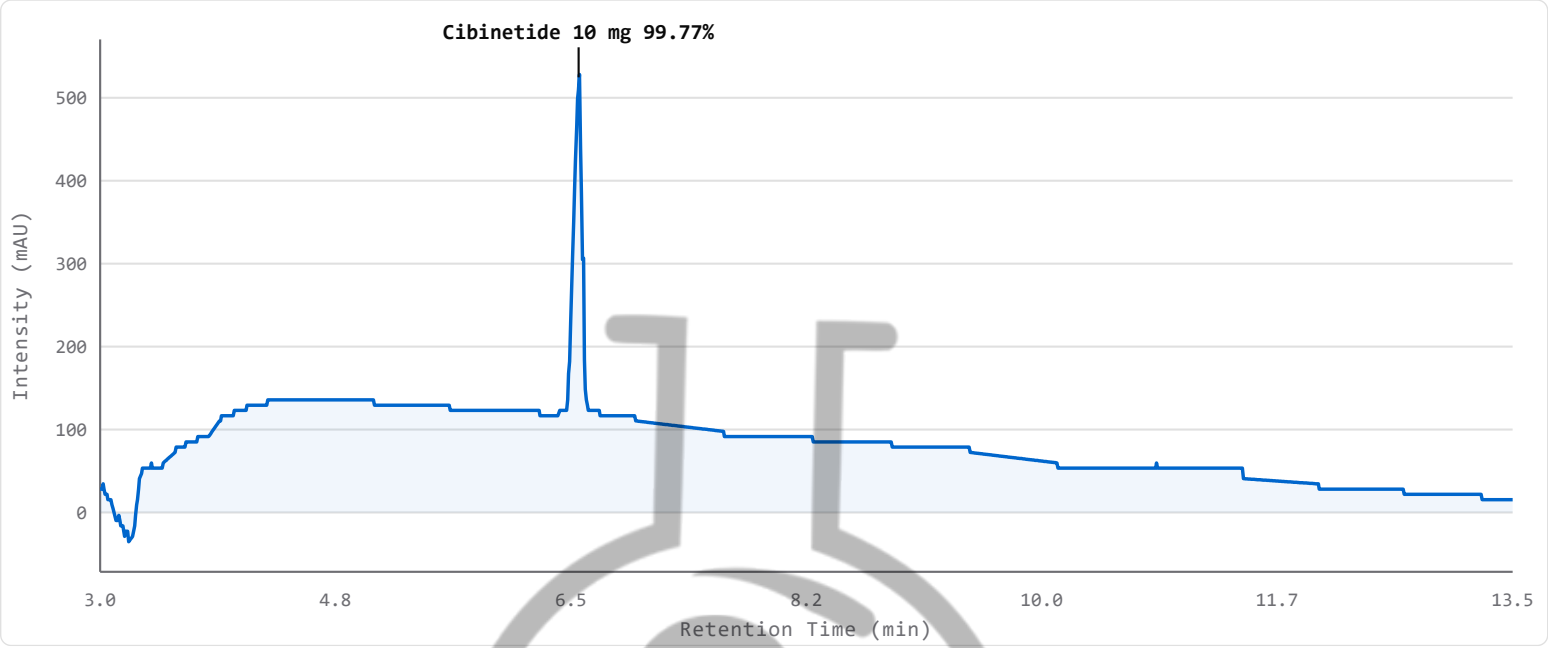


*Representative chromatogram (n=3). Identification by retention-time comparison with a reference standard.*

PASS - Endotoxins <0.05 EU/mg; PASS - No microorganisms present in sample tested; Chromatographic Purity >99.80% + 0.18%; Assay 10.80 mg; Heavy metals ND. Microbiology: Pass.

Corey Klein

Corey Klein
LABORATORY TECHNICIAN
2026-09-07

**Issued** 2026-09-08 **Revision** 1.0 **Record hash (SHA-256)** 9a9181f5169f8a8c102b0fde1b25b36d367c8818627fb902554452f71642fcf9

Samples were received in acceptable condition. The result(s) in this report relate only to the portion of the sample(s) tested. All analyses were performed consistent with the Verum Analytical Quality Management System. Verum Analytical and its staff did not observe or participate in the sample selection process, and cannot confirm the authenticity of the sample or its representativeness of the associated lot/batch. Results apply only to the tested sample(s) as received. Results relate only to the sample as received. Verifiable at source at verify.verumanalytical.com